


# PILOT 12/24 CONTROL PANEL GUIDE

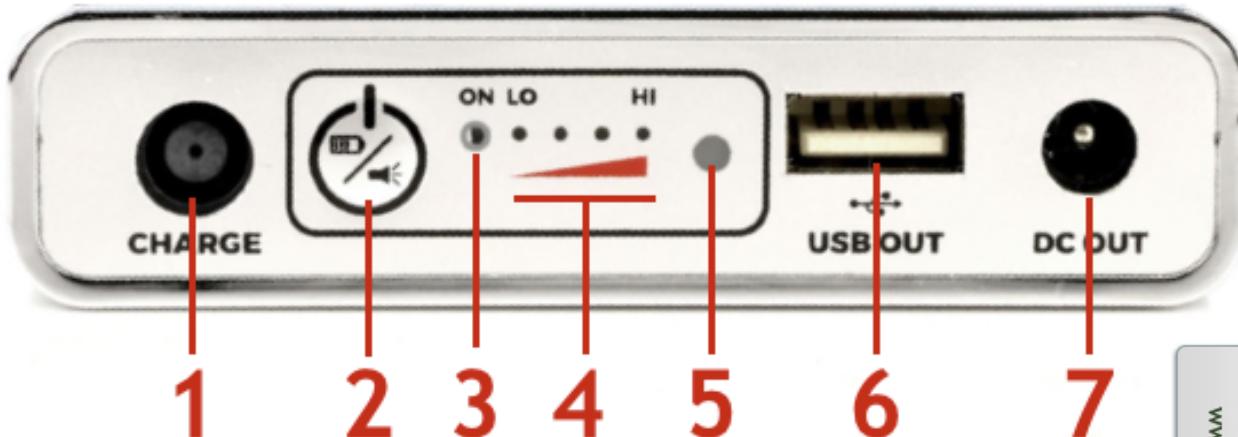

## 1. AC Charge Port

- Use the PAP machine's AC power cord to charge battery
- Leave AC Power Cord connected for use as a Backup Power Source.

## 2. Multi Function Button

- TAP button to display charge level indicator (GREEN LED's)
- HOLD button to activate / deactivate LED FLASHLIGHT

## 3. Blue "ON" Indicator Light (LED)

- The BLUE LED will activate when connected and sending power to a device.

## 4. Green Charge Level Indicator Lights (LED)

|                         |                              |
|-------------------------|------------------------------|
| 4 Solid Green Lights    | $\geq 90\%$ charge remaining |
| 3 Solid Green Lights    | 65% - 90% charge remaining   |
| 2 Solid Green Lights    | 40% - 65% charge remaining   |
| 1 Solid Green Light     | 10% - 40% charge remaining   |
| 4 Flashing Green Lights | Battery is CHARGING          |

## 5. Flashlight (LED)

## 6. USB Port (5V, 2.5A Out)

- Used for charging handheld devices.
- Once a USB cable is connected, tap the "Multi Function Button" (no. 2) to activate battery.

## 7. DC Out Port

- This port is used to connect a compatible PAP device to the battery

Presented With Compliments From  
[www.DirectHomeMedical.com](http://www.DirectHomeMedical.com)

